


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

022 2009

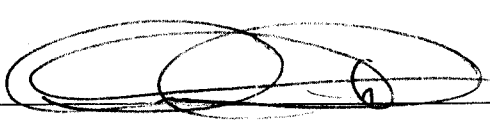Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	30292
Name	ANDRE ACHEE	ID#	2385 Date 9-15-09
Agency	BETHEL POLICE DEPT	Phone #	907-543-3781
Instrument Location	BPD SQUAD ROOM		
Alco S/N	X124650	Target Value	.086
		High Pressure	250 PSI
Alco Test Values	.084	.084	
	1 st Alco	2 nd Alco	
Signature			
(OVER)			

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz

Scientific Director


State Breath Alcohol Program

Subscribed and sworn before me this 6th day of NOV., 2009.

Carolyn M. Noland

Notary Public, State of Alaska

Commission Expires with Office

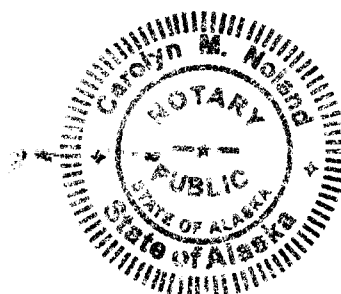

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130292

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130292

SEPTEMBER 15, 2009

OPERATOR'S NAME:

ACHE/ANDRE/A

OPERATOR'S NUMBER: 2385

SUBJECT'S LAST NAME:

TEST

SUBJECT'S FIRST NAME/MI :

UOC

O.L. #: 1234567

DEPT/AGENCY: BET1

CASE/REPORT: XXXXXXX

TEST TYPE: T

ALCO TARGET VALUE: .086

ALCO S/N: K124650

--- BREATH ANALYSIS ---

.086 ADJUSTED FOR 30.11 in
ALCO TARGET .086 14:46
BLANK TEST .000 14:46
INTERNAL STANDARD VERIFIED 14:46
ALCO TV 30.11 in .084 14:47
BLANK TEST .000 14:47
SUBJECT SAMPLE .000 14:48
BLANK TEST .000 14:48
ALCO TV 30.11 in .084 14:49
BLANK TEST .000 14:49

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130292

SEPTEMBER 15, 2009

TIME 14:44

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 01/08/09
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 40c
BAROMETER: 30.11 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~